




SENSAR® 1-Piece Hydrophobic Acrylic IOL

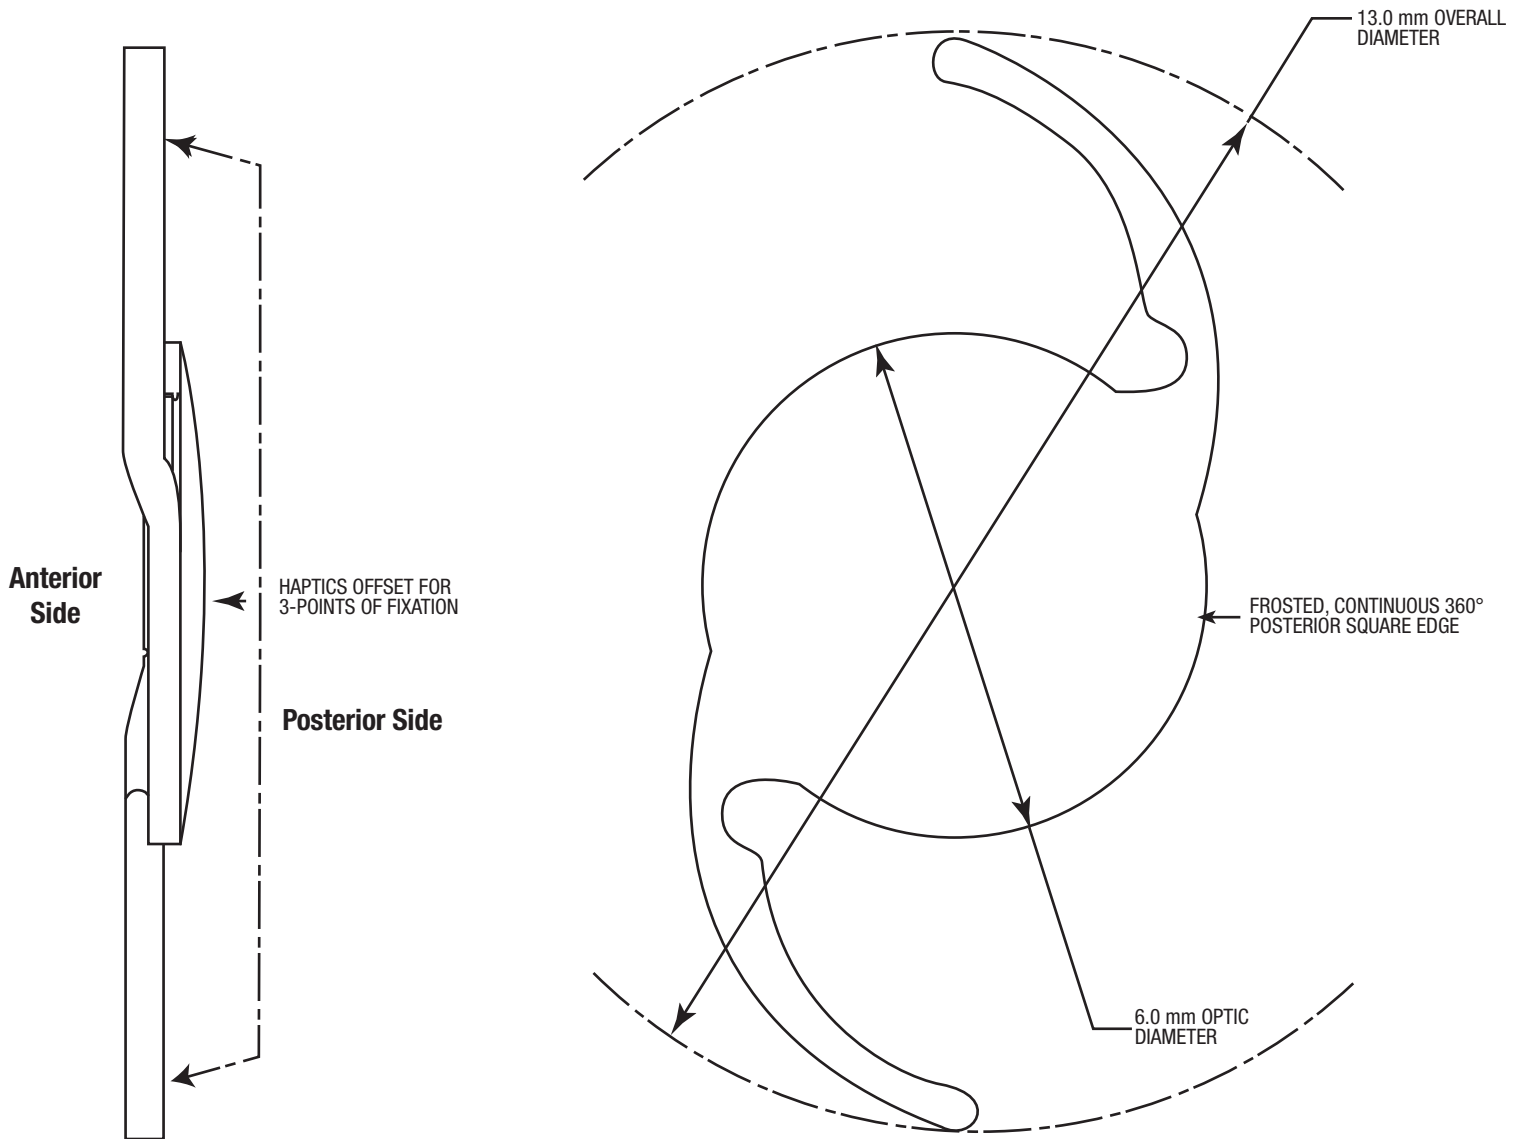

DESCRIPTION	
OPTIC CHARACTERISTICS	
Powers:	+6.0 D to +30.0 D in 0.5 diopter increments
Diameter:	6.0 mm
Material:	UV-blocking hydrophobic acrylic
Refractive Index:	1.47
Edge Design:	ProTEC frosted, continuous 360° posterior square edge
ULTRASOUND BIOMETRY*	
A-constant:	118.4
Theoretical AC Depth:	5.2 mm
Surgeon Factor: ¹	1.45 mm
HAPTIC CHARACTERISTICS	
Overall Length:	13.0 mm
Style:	C
Material:	UV-blocking hydrophobic acrylic
Design:	Haptics offset from optic
RECOMMENDED INSERTION INSTRUMENTS	MODEL
UNFOLDER® Platinum 1 Series Handpiece	DK7796
UNFOLDER® Platinum 1 Series Cartridge	1MTEC30
One Series Ultra Implantation System (Syringe-style Inserter)	DK7786
One Series Ultra Implantation System (Screw-style Inserter)	DK7791
One Series Ultra Cartridge	1VIPR30

*Value theoretically derived for a typical 20.0 D lens. AMO recommends that surgeons personalize their A-constant based on their surgical techniques and equipment, experience with the lens model, and postoperative results.

**To learn more and to view important safety information,
please contact your AMO Sales Representative.**

AMO United Kingdom Limited • Jupiter House • Mercury Park • Wycombe Lane
Wooburn Green • High Wycombe • Buckinghamshire • HP10 0HH • UK

1. Calculated based on Holladay I formula (Holladay JT, Prager TC, Chandler TY, Musgrove KH, Lewis JW, Ruiz RS. A three-part system for refining intraocular lens power calculations. *J Cataract Refract Surg.* 1988;14(1):17-24).

SENSAR® 1-piece lenses are indicated for the visual correction of aphakia in adult patients in whom a cataractous lens has been removed by extracapsular cataract extraction. These devices are intended to be placed in the capsular bag. For a complete listing of precautions, warnings, and adverse events, refer to the package insert.

One Series, SENSAR®, ProTEC and UNFOLDER® are trademarks owned by or licensed to Abbott Laboratories, its subsidiaries or affiliates.

©2011 Abbott Medical Optics Inc., Santa Ana, CA 92705 www.AbbottMedicalOptics.com

2011.11.14-CT4255